


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


JUL 07 2009

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130299 -
Name		Christopher M Babcock	ID# 3867 Date 7-1-09
A	Agency	King Cove Dept. Public Safety	Phone # 497-2210
Instrument Location		Squad Room	
Alco S/N		75603 75260	Target Value .078 High Pressure 1200
B	Alco Test Values	.081 1 st Alco	.082 2 nd Alco
Signature			
(OVER)			


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 20th day of July, 2009.

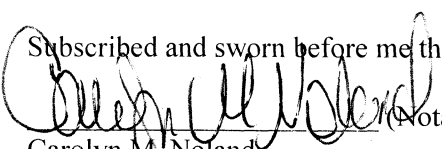
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

130299 ✓

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

[illegible]